


PROTON DMSO D:\ nmr1 20

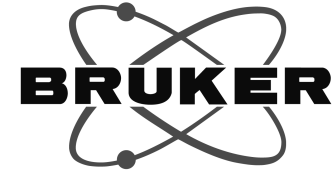

Current Data Parameters
NAME A-1400
EXPNO 10
PROCNO 1


F2 - Acquisition Parameters
Date_ 20190909
Time 11.03
INSTRUM spect
PROBHD 5 mm PABBO BB-
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.122266 Hz
AQ 4.0894465 sec
RG 101
DW 62.400 usec
DE 6.50 usec
TE 311.2 K
D1 1.00000000 sec
TD0 1

==== CHANNEL f1 =====
SFO1 400.1324710 MHz
NUC1 1H
P1 14.00 usec
PLW1 20.00000000 W

F2 - Processing parameters
SI 65536
SF 400.1300000 MHz
WDW no
SSB 0
LB 0 Hz
GB 0
PC 1.00

10.133
8.039
8.017
7.958
7.936
7.521
7.514
7.307
7.301
7.285
7.279
6.804
6.798
6.782
6.776
6.724
6.718

3.480
2.545
2.511
2.507
2.502

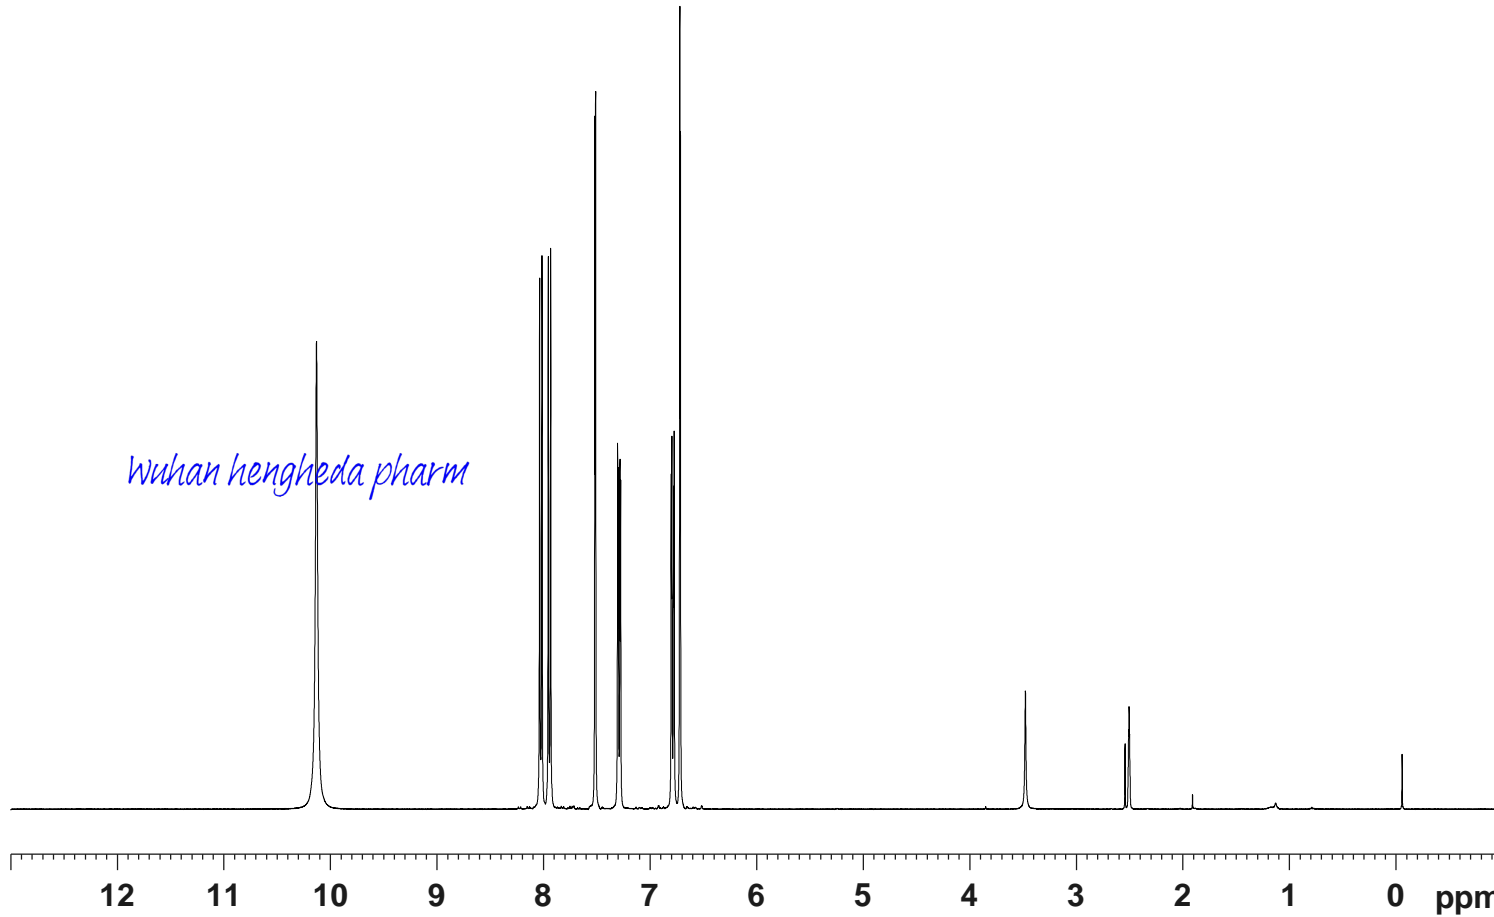

2.01
1.00
0.99
1.00
1.01
0.99
0.99