



Nucleic Acid (Throughput-96) Automatic Extraction System



Nucleic Acid Automatic Extraction System (Throughput-96)

Product introduction: With the latest isolation method of nucleic acid transferred by magnetic rods and preloaded magnetic beads-based extraction reagent, The YC796 Nucleic Acid Automatic Extraction System can process 1-96 samples and automatically isolate nucleic acids from various samples such as blood, cells, viruses, etc. The magnetic beads are adsorbed, transferred and released by the special magnetic rod, so as to realize the fully automated purification of nucleic acid.

【Product Features】




	Strong magnetic force 5500 Gauss magnetic rod ensure magnetic beads recovery rate ≥98%		Programming In addition to programed protocols, support customers to create and edit protocols to meet the diverse needs
	Small size It can be placed in a common biological safety cabinet		Precise temperature control Automatic heating for lysis and elution, with fast heating speed and precise temperature control
	Avoid cross contamination Intelligent magnetic rod motion control system and UV sterilization module effectively reduce the cross contamination between wells		Door opening protection The program automatically pauses when opening the door in the working state, and automatically continues after closing
	Open system Applicable to various magnetic beads-based extraction reagents		Short operating time Complete the nucleic acid extraction of 96 samples within 30 minutes

Nucleic Acid Automatic Extraction System (Throughput-96)


[Unique Magnetic Rod Movement]

The driving device is equipped with a high-performance stepping motor, with large magnetic rod vibration amplitude. The vibration amplitude can be set according to the volume of the solution to ensure good and even blending effect. The actuator is made of ball screw to ensure that the rod runs smoothly, has high precision and long service life. Each moving component is protected by the limit position protection mechanism to avoid instrument failure.

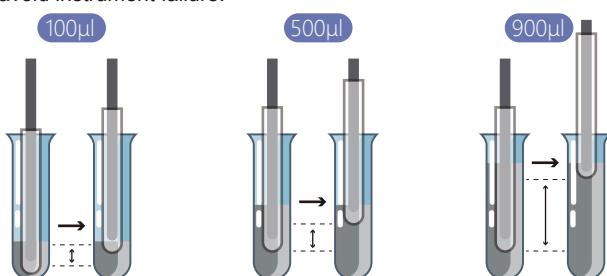


[New Strong Magnetic rod]

With the newly designed strong magnetic rod, the magnetic beads are absorbed on the head of the magnetic rod, so as to ensure that the elution buffer can still cover all the magnetic beads even with a small elution volume. The high recovery of magnetic beads ensures high yield of nucleic acid.

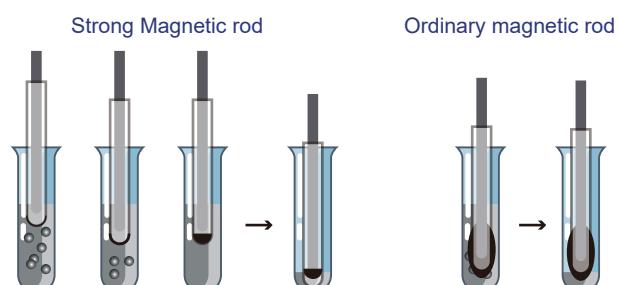

[Working principle]

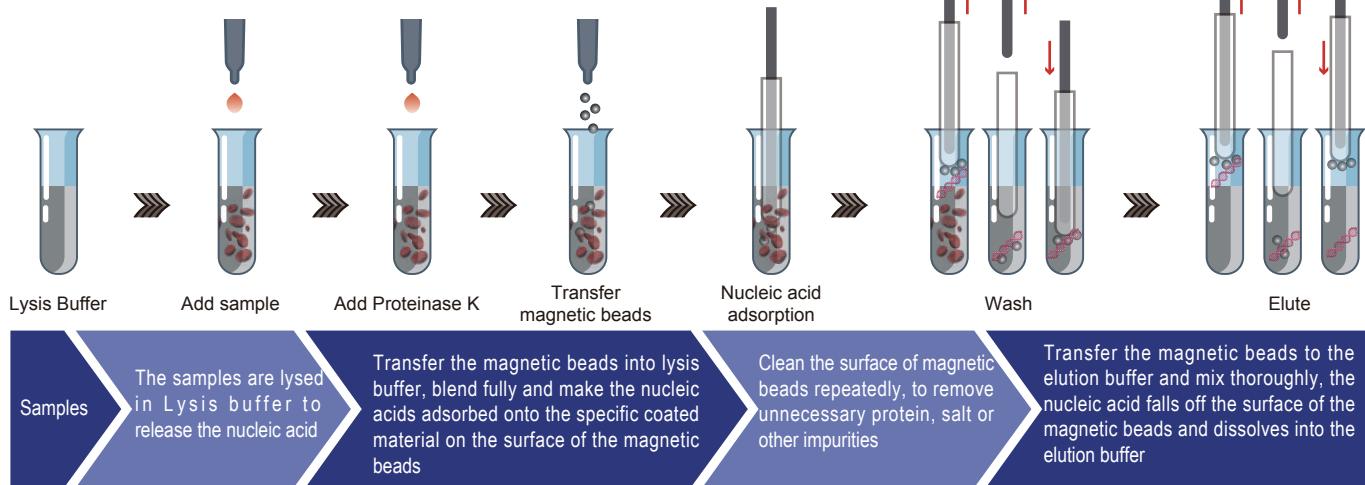

[Instrument parameters]

Product name	Nucleic Acid Automatic Extraction System	
Model	YC796	Ambient temperature ~95°C
Certification	CE/ RoHS	Nucleic acid extraction purity 1.8≤OD260/OD280≤2.0
Extraction channel	1-96	Inter-well purification variation CV<3%
Consumables	96 well plate + Tip comb	Magnetic beads recovery ≥98%
Nucleic acid extraction time	15-35 minutes	Touch screen size 7 inch color touch screen
Temperature control precision	0.5°C	Disinfection/decontamination method UV
Temperature control accuracy	±1.5°C	Input power AC 100-240V~, 3.4A, 50Hz
Temperature uniformity	±1.0°C	Product weight 52±1kg
		Product size 743mm*465mm*447mm

Nucleic Acid Automatic Extraction System (Throughput-96)

【Kits and reagents】



The kit is suitable for TECHSTAR YC769 Nucleic Acid Automatic Extraction System for extracting genomic DNA/RNA of pathogenic microorganisms from samples such as serum, plasma, cultured cells, saliva, alveolar lavage fluid, nasopharyngeal aspirates and swabs.

【Product name】

Magnetic Bead-Based Nucleic Acid (DNA/RNA) Extraction Kit

【Product No.】

SC905

【Packing specification】

96 T/Kit

【Transportation condition】

Room temperature

【Preservation condition】

Room temperature, or 2-8°C for long-term preservation

【Period of validity】

12 months

【Applicable instrument】

TECHSTAR YC796 Nucleic Acid Automatic Extraction System

【Features】

Reliable stability

Unique "Protease K" stable at room temperature, the complete kit does not need to be stored at low temperature.

High binding

Magnetic beads optimized for pathogenic microbial genomes have excellent adsorption effects on small nucleic acids.


Strong sealing

High-viscosity sealing film prevents liquid leakage during transportation.

High sensitivity

With strong reproducibility and high purity, it can recover trace amounts of pathogenic microorganism DNA/RNA.

【Operation procedures】



Tear off the sealing film

Add sample and Proteinase K

Loading to the instrument



Nucleic acid extraction

Nucleic Acid Automatic Extraction System (Throughput-96)



【Product components】

Name	Quantity	Capacity	Components
Tip comb	1	/	/
Sample plate	1	500µL×96	Guanidine Hydrochloride, TritonX-100, EDTA, etc.
Beads plate	1	200µL×96	Magnetic beads
Wash 1 plate	1	600µL×96	Guanidine Hydrochloride, EDTA, etc.
Wash 2 plate	2	600µL×96	75% ethanol
Elution plate	1	100µL×96	TE buffer
Protease K	1mL x 2	/	Protease K



【Dimensions】

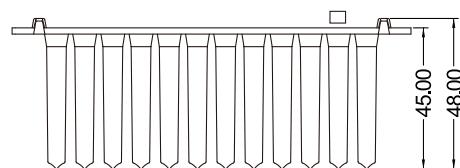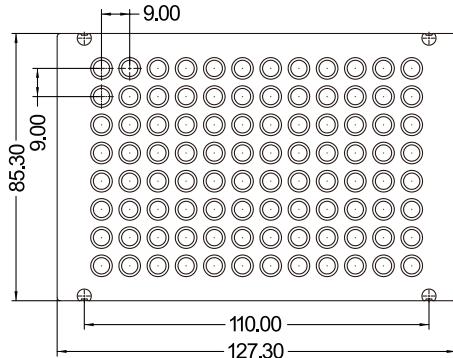


Tip comb

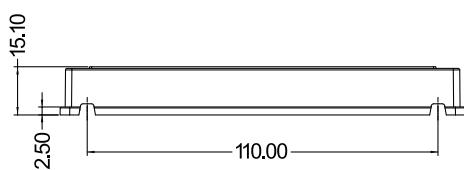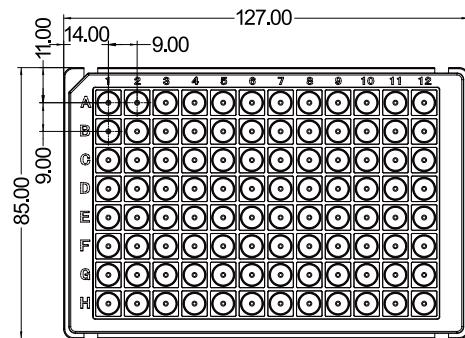

96 standard plate

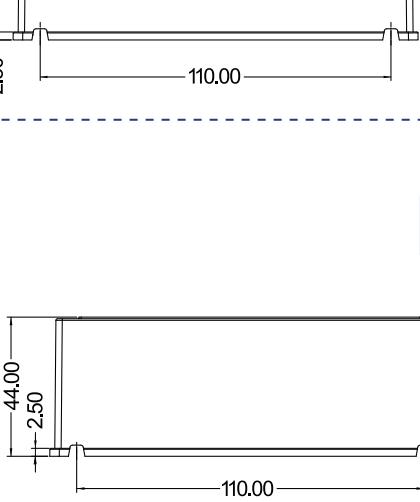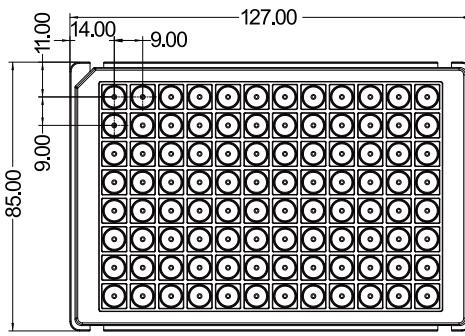

96 deep-well plate

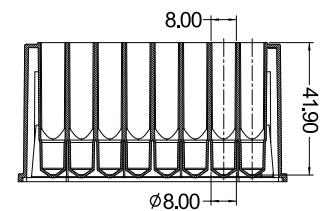



techstar | Wuxi Techstar Technology Co.,Ltd.
📍 Workshop 2, No.117, Meiyu Road,
Meicun Street, Xinwu District, Wuxi, Jiangsu, PRC

☎ +86-18915343062

🌐 www.tech-star.cn

✉ sale06@tech-star.cn