

Sample Collection Set

The sample collection set is used for storage and transportation of human specimen. It offers biological buffer, maintains normal PH value of organism and stability of nucleic acid and prevents nucleic acid degradation. Besides, the product can inactive the advanced structure of pathogen protein, deprive biological activity and reduce infectivity and pathogenicity.



Stable

prevent nucleic acid degradation



Safe

inactivated,reduce infectivity and pathogenicity




Parameters

Specification	10T/Kit
Product Code	T319H
Specimen Collection Method	Nasopharyngeal swab or Oropharyngeal swab
Storage and Stability	Store under room temperature; Validity period:12 months
Usage	Storage and transportation of human specimen


Test Procedure




① Swab on the posterior wall of the pharynx tonsil recess, lateral wall,etc. Repeatedly wipe 3-5 times.

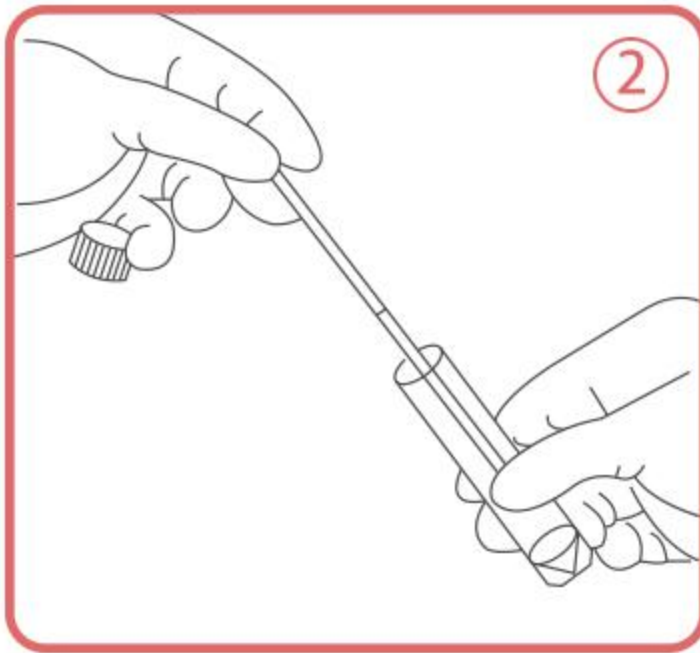

② Immerse the swab head after sampling preserved in liquid in the tube.

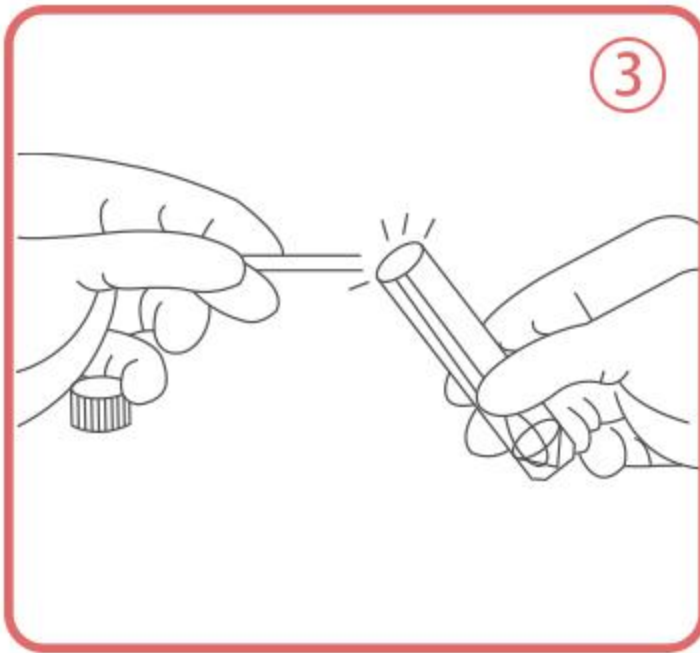

③ Break off the swab from the breaking point

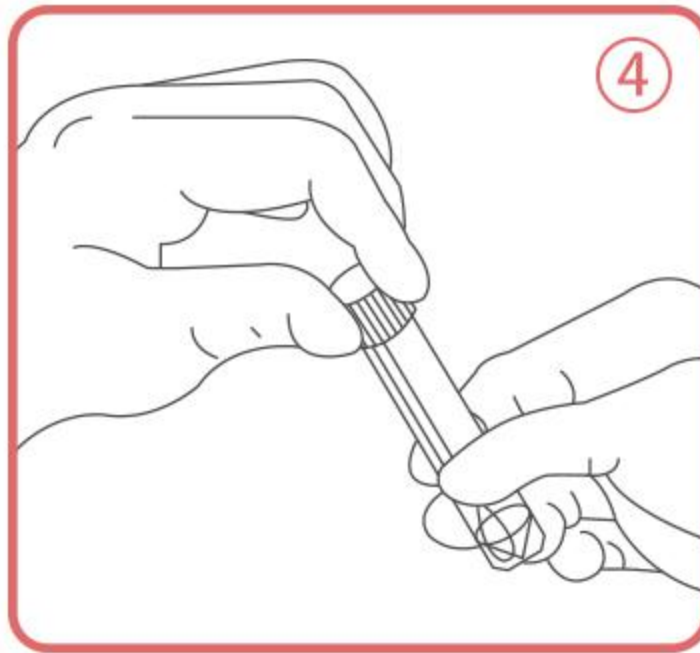

④ Tighten the lid and shake



Tianlong Biotech

Mail: inquiry@medtl.com
Phone: 86 029 82682132
website: www.tlgenetech.cn
Address: No. 389 Zhuhong Road,Xi'an, China

Sample Collection Set

The sample collection set is used for storage and transportation of human specimen. It offers biological buffer, maintains normal PH value of organism and stability of nucleic acid and prevents nucleic acid degradation. Besides, the product can inactive the advanced structure of pathogen protein, deprive biological activity and reduce infectivity and pathogenicity.



Stable

prevent nucleic acid degradation



Safe


inactivated,reduce infectivity and pathogenicity




Parameters

Specification	48T/kit		
Product Code	T326H	T326HB	T326HC
Specimen Collection Method	Oropharyngeal swab	Nasopharyngeal Swab	Nasopharyngeal swab & Oropharyngeal swab
Storage and Stability	Store under room temperature; Validity period:12 months		
Usage	Storage and transportation of human specimen		


Test Procedure

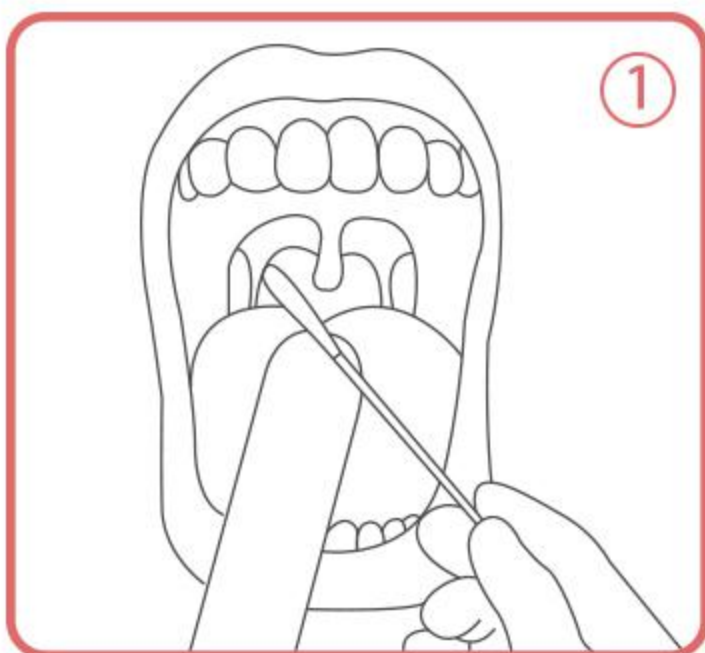


① Swab on the posterior wall of the pharynx tonsil recess, lateral wall,etc. Repeatedly wipe 3-5 times.

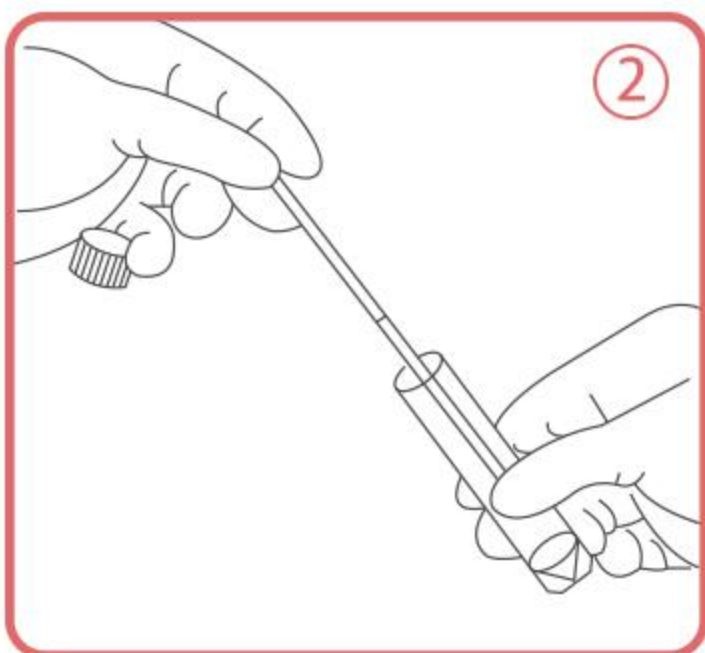

② Immerse the swab head after sampling preserved in liquid in the tube.

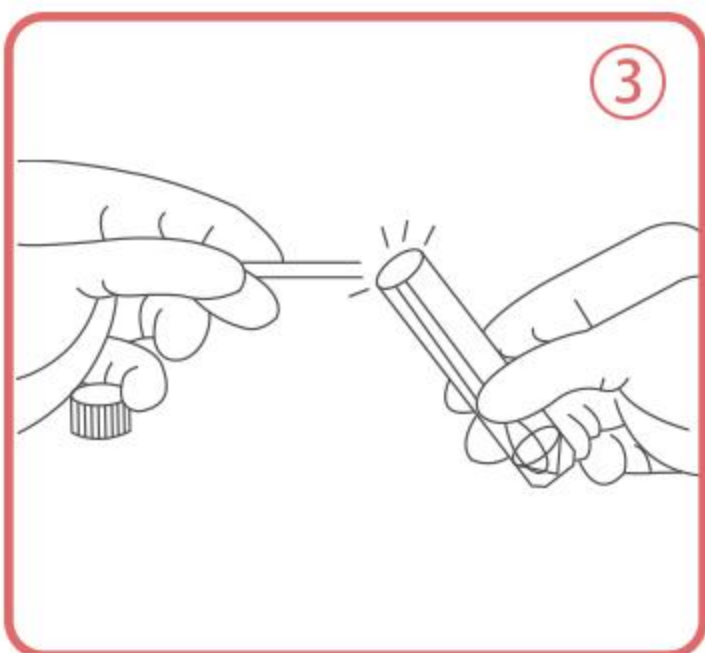

③ Break off the swab from the breaking point

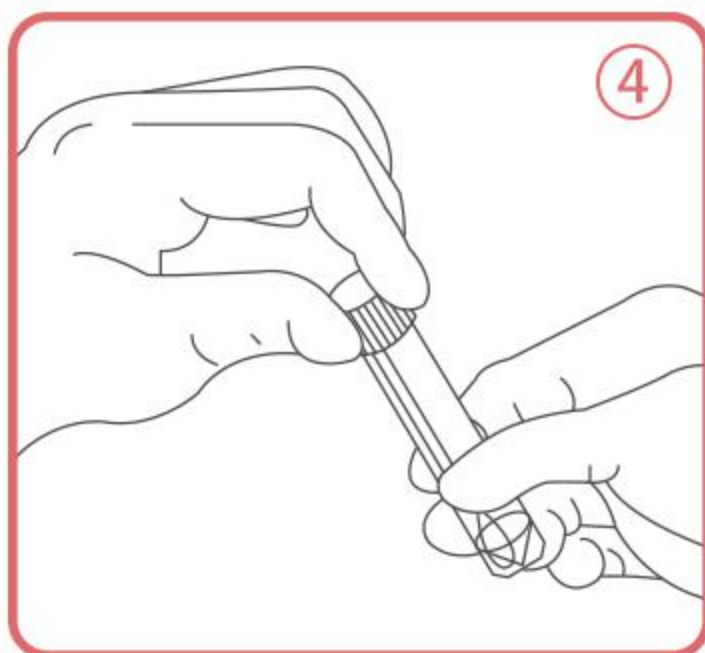

④ Tighten the lid and shake



Tianlong Biotech

Mail: inquiry@medtl.com
Phone: 86 029 82682132
website: www.tlgenetech.cn
Address: No. 389 Zhuhong Road,Xi'an, China